

Flavonoids

Experimental

Column: SVEA Core C18, 2.6 μ m, 4.6*100mm

Instrument: HPLC


Flow rate: 1.0 mL/min

Column temperature: 40 °C


Detector: UV 260 nm

Sample:
1 Myricetin
2 Quercetin
3 Apigenin
4 Baicalein


Mobile phase: Methanol/water/formic acid (50/50/0.1)

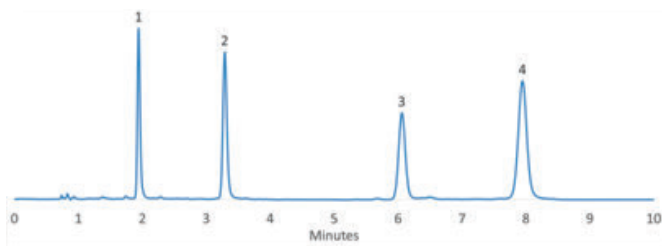

Mobile phase: Acetonitrile/10mM phosphoric acid (35/65)

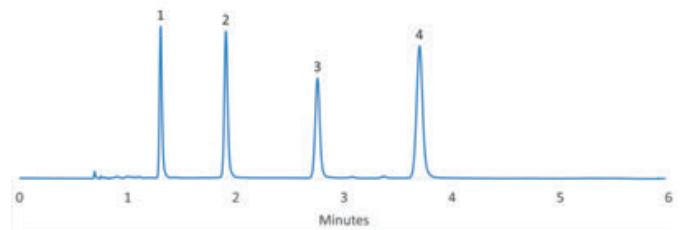

Mobile phase: Methanol/10mM phosphoric acid (50/50)

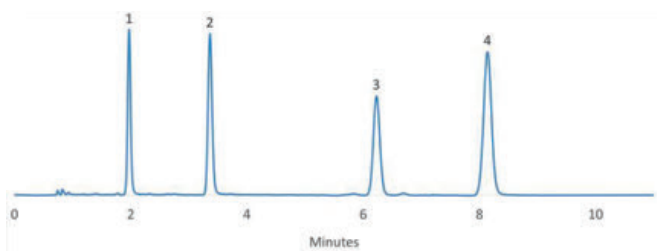

Mobile phase: Acetonitrile/water/formic acid (35/65/0.1)

